Diagnostic Instructions

Mobile Stand Assembly Instructions Model 48850

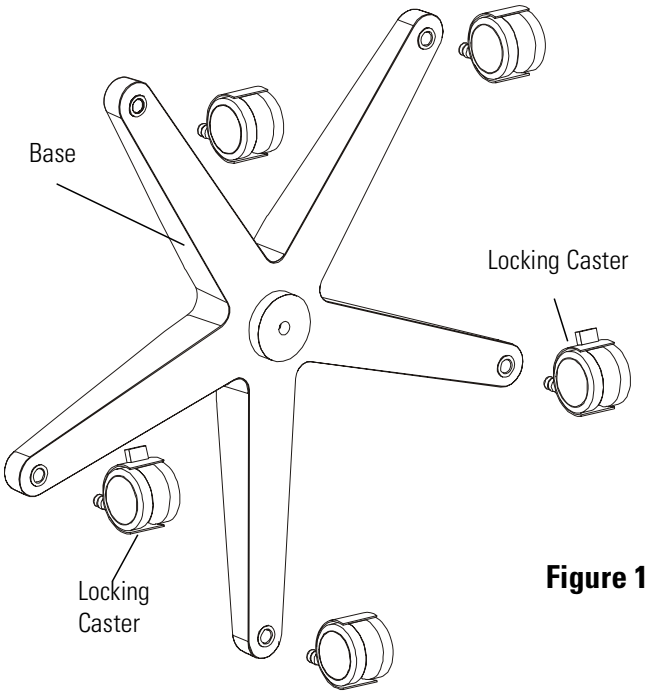

Figure 1

Components

- Column (1)
- Base (1)
- Locking Casters (2)
- Non-Locking Casters (3)
- .25 inch (.64 cm) Lock Washer (1)
- .75 inch (1.9 cm) Flat Washer (1)
- Socket Head Bolt (1)
- Hex Socket Wrench (1)
- .50 inch (1.27 cm) mounting screws (2)

Caster/Base Assembly Instructions (figure 1):

Push casters into the holes of the base until they "snap" into place. Alternate casters as shown.

Base/Column Assembly Instructions (figure 2):

1. Insert column into center hole of base.
2. Insert .25 inch (.64 cm) lock washer, .75 inch (1.9 cm) flat washer and 1 1/4" (3.2 cm) socket head bolt into center hole. Tighten socket head bolt with hex socket wrench.

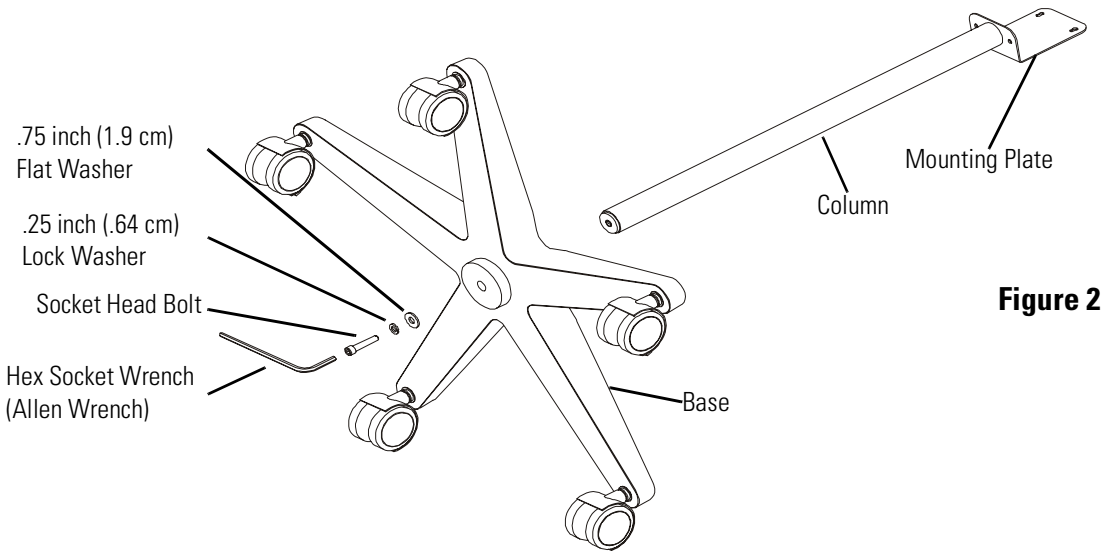

Figure 2

Exam Light/Mounting Plate Instructions, see reverse.

Exam Light/Mounting Plate Instructions (figure 3):

1. Place the keyhole pins on the back of the Exam Light into the slots on the top of the mounting plate and slide down.
2. Line up the screw holes on the bottom of the Exam Light with the screw holes on the mounting plate .
3. Insert the .50 inch (1.27 cm) screws through the bottom of the mounting plate and tighten with a phillips head screw driver (not included).

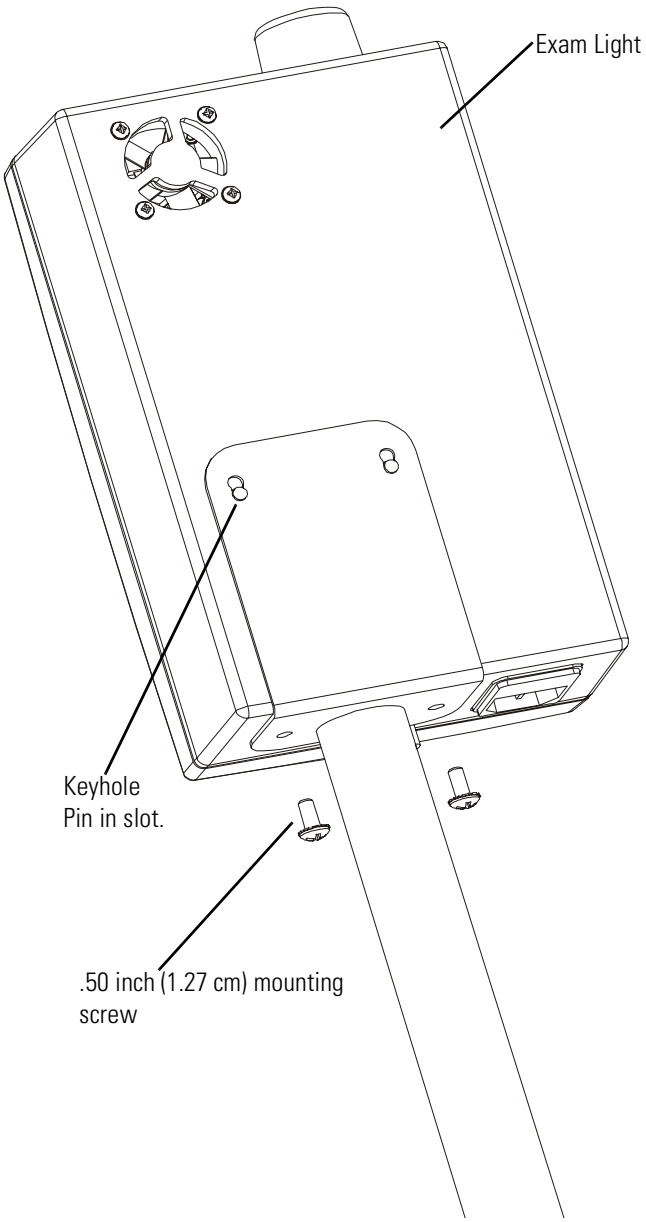

Figure 3

Welch Allyn®

Welch Allyn, Inc.
4341 State Street Road
PO Box 220
Skaneateles Falls, New York 13153-2002 USA
Telephone: (315) 685-4560
Fax: (315) 685-3361